




REPLACEMENT SHEET DRAWING

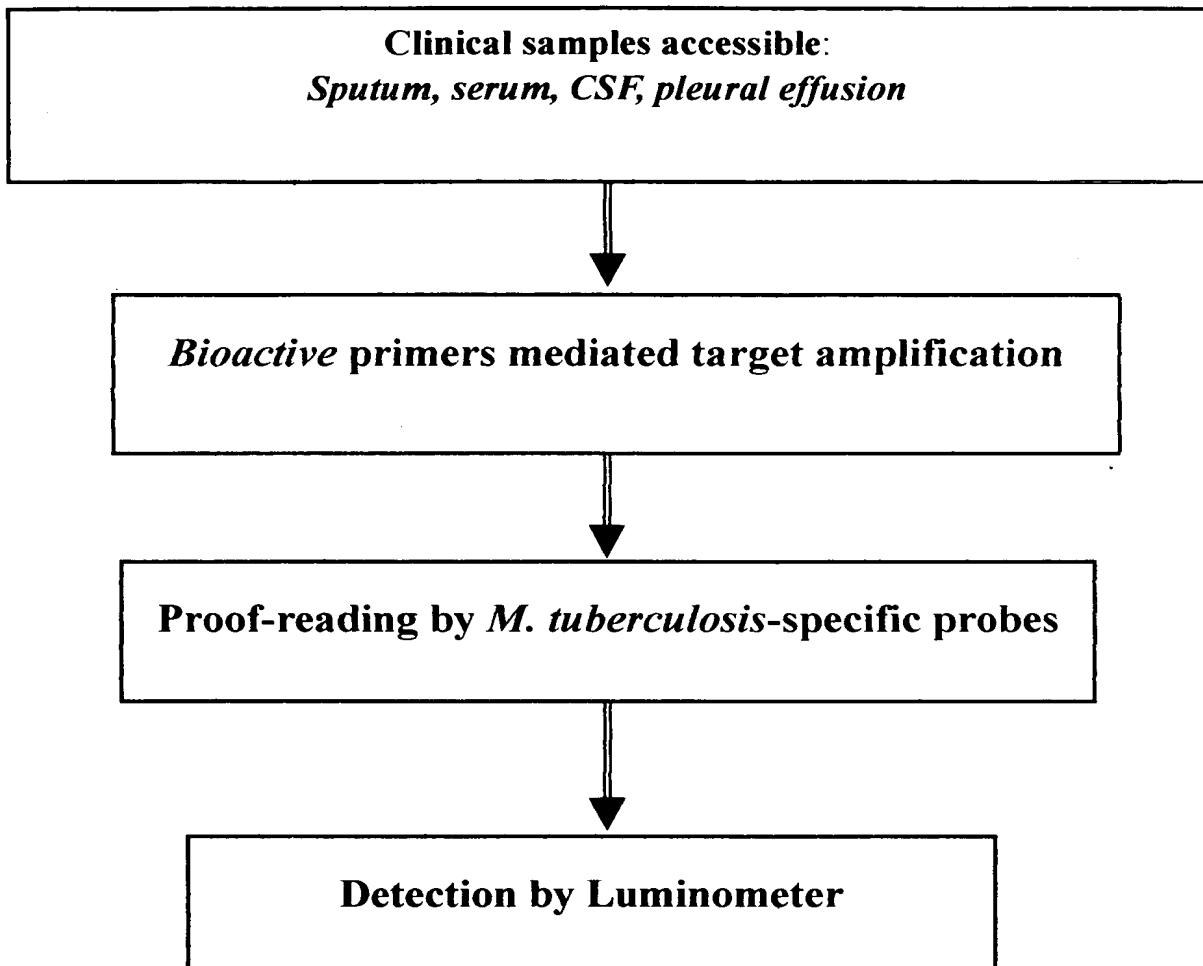

(Whole process < 5 hours)

FIG. 1

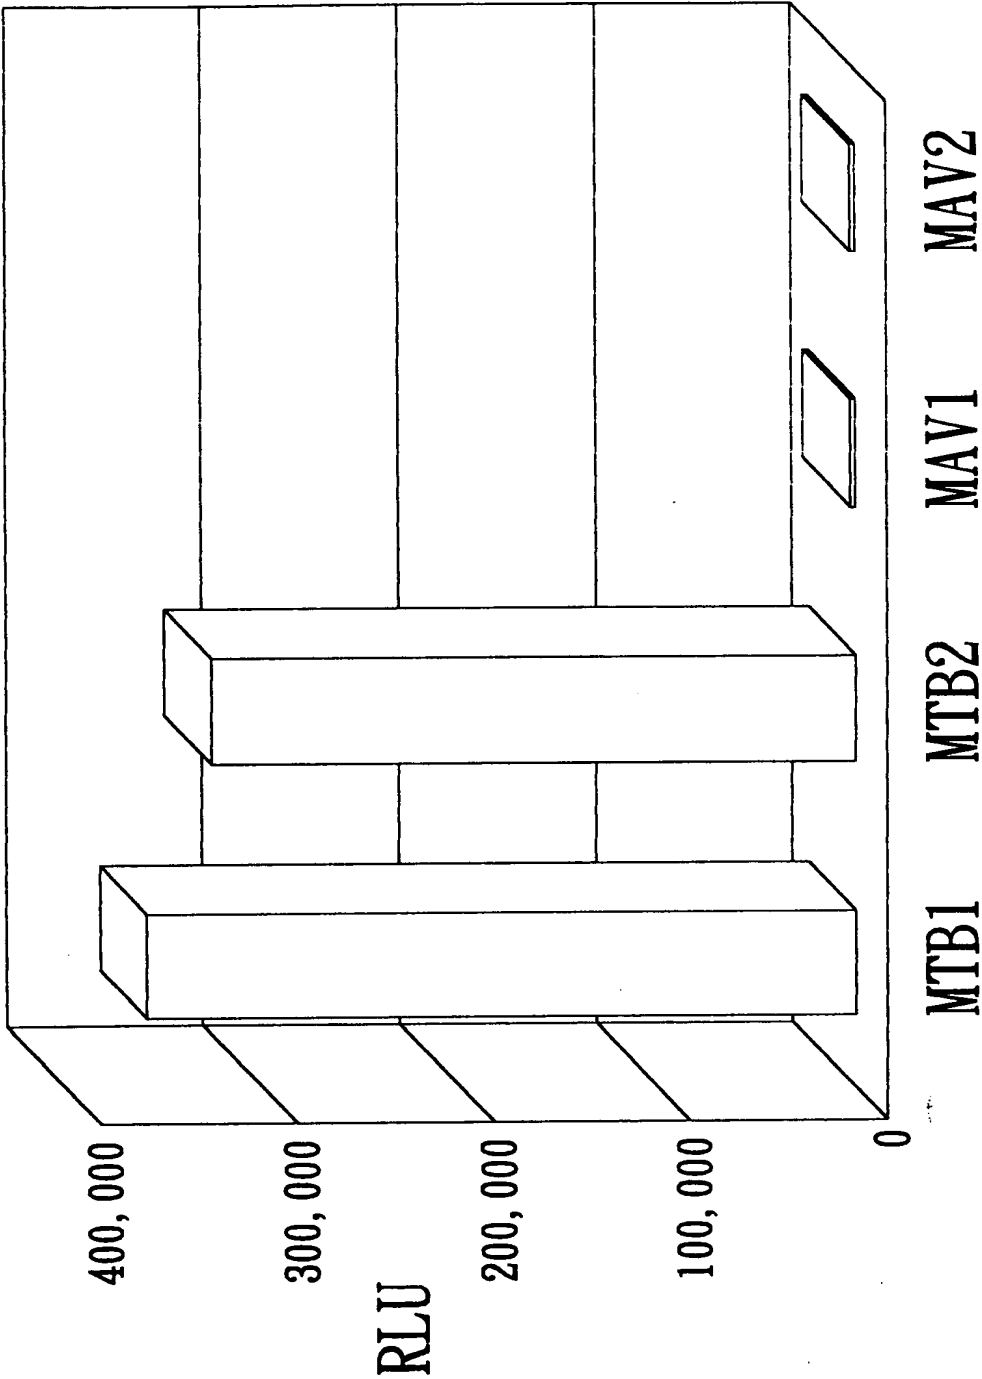


FIG. 2

REPLACEMENT SHEET DRAWING

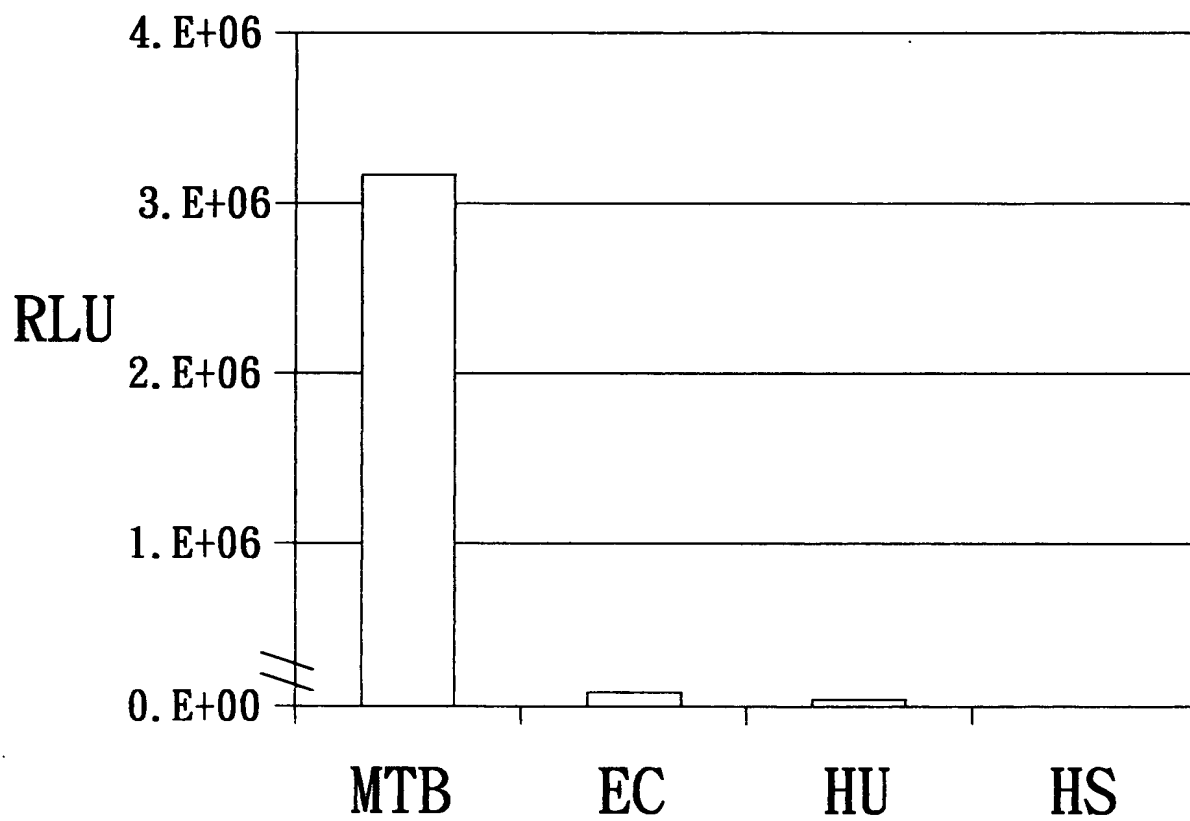


FIG. 3

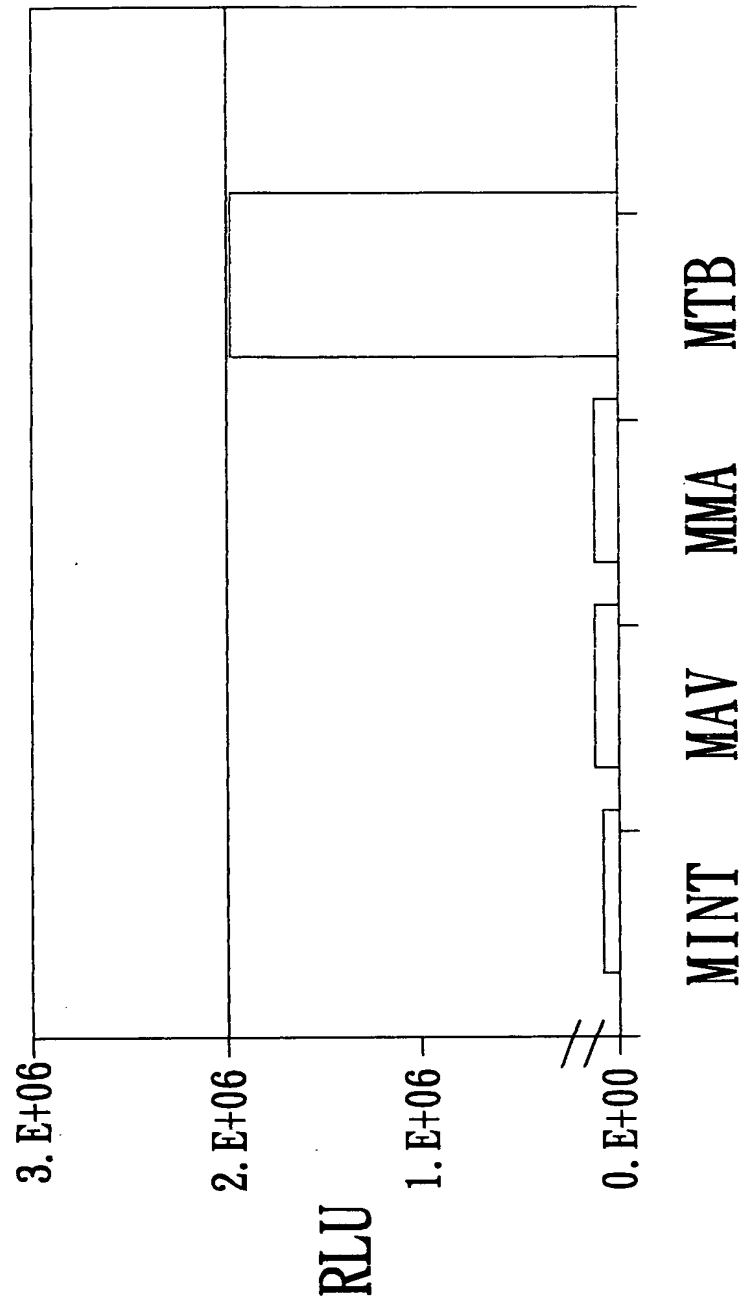


FIG. 4

Standar*	AsiaGe MT Detection Kit		Sensitivity = 100% Specificity = 100%
	+	—	
+	32	0	32
—	0	73	73
	32	73	105

PPV = 100% NPV = 100%

Smea⁺, Culture⁺, Nested PCR⁺
 PPV: Positive Prediction
 NPV: Negative Prediction Value

FIG. 5

REPLACEMENT SHEET DRAWING

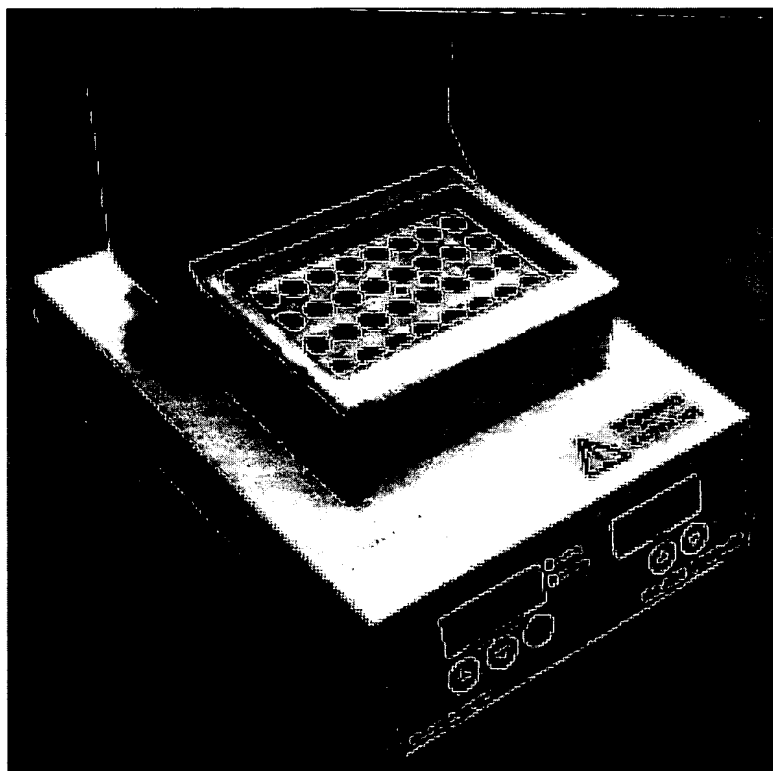


FIG. 6